Environmental Monitoring With An Electrochemical Whole-Cell Based Biochip Sensor: As(III) In Tap Water

Fernando Cortés Salazar, 1 Siham Beggah, 2 Jan Roelof van der Meer 2 and Hubert Girault. 1

¹Ecole Polytechnique Federale de Lausanne (EPFL); ²Université de Lausanne (UNIL). Lausanne, Swtizerland.

1. INTRODUCTION

The development of an electrochemical sensor for living cell toxicity detection by coupling biological engineering and electrochemical techniques is presented. In presence of a toxic agent many different bacteria develop a natural resistance mechanism based on the selective detection of the toxic species and its pumping out from the cell (e.g. E.coli has a natural resistance to As(III)).1 Therefore, toxic effects in bacteria can be accurately detected when coupling a genetically modified signaling cascade to the toxicity mechanism. Such 'reporter bacteria' can produce a measurable signal, which can be read out by various means such as electrochemistry.^{2,3} Here we describe the use of a genetically engineered *E. coli* for detecting low arsenic concentrations in tap and ground water from Switzerland with a microchip containing 16 individually addressed electrochemical cells for high-throughput environmental monitoring of arsenic in potable water. The main advantages of the present approach over previously reported arsenic bacterial bioreporters are the faster response time and the higher sensitivity achieved (LOD = 0.8 ppb).

2. PRINCIPLE OF As(III) BIOSENSING AND ELECTROCHEMICAL DETECTION

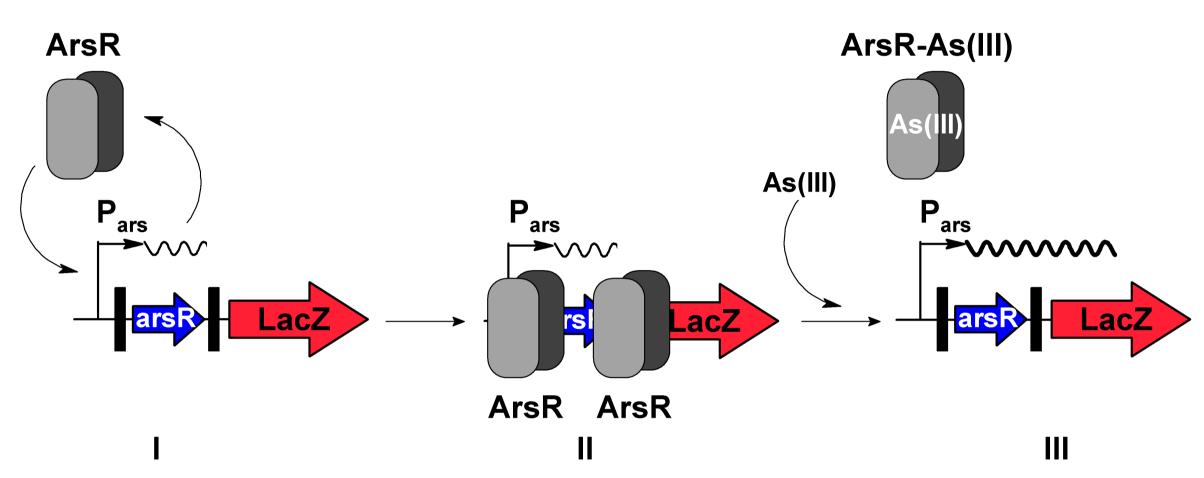


Figure 1. Principle of the As(III) bioreporter. I) The ArsR repressor protein (sensing protein) is synthesized from the arsR promoter (Pars). II) ArsR binds to two binding sites on the DNA and prevents expression of the reporter gene (LacZ) and the subsequent formation of beta-galactosidase (β-Gal). III) When As(III) is present, ArsR loses its affinity for the binding sites on the DNA and the transcription of the arsR and LacZ genes takes place and as a consequence β-Gal is synthesized. The activity of the expressed β-Gal can be detected by following the product of its reaction (p-aminophenol, PAP) with p-aminophenyl galactopyranoside (PAPG).¹

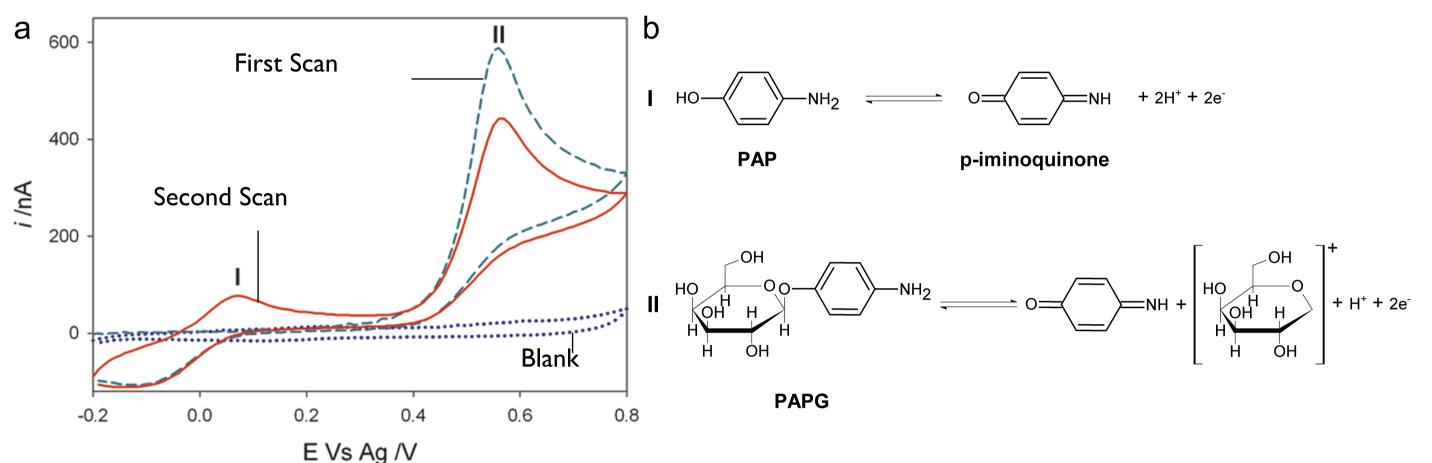
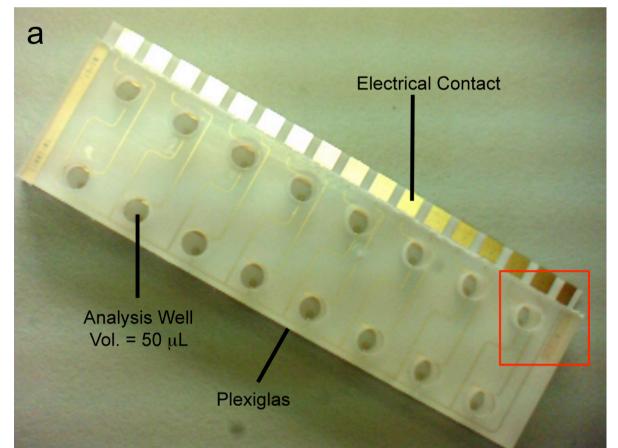


Figure 2. Electrochemical monitoring of PAP. a) Cyclic voltammetry of PAPG 1 mM in PBS 1x (pH = 7), first scan (cyan dashed line), second scan (red continuous line) and supporting electrolyte PBS 1x (blue dotted line). Scan rate = 20 mV/s. b) Electrochemical reactions taking place at I (i.e. PAP oxidation) and II (i.e. PAPG oxidation).4 By working at a constant potential of 0.05 V Vs Ag, the production of PAP can be monitored electrochemically.

3. EXPERIMENTAL SETUP AND PROTOCOL




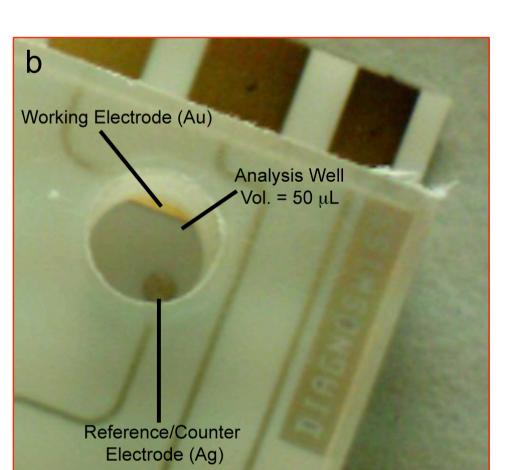


Figure 3. a) Optical photography of the microchip employed for the stop flow measurements of As(III). The microchip contains 16 independent electrochemical sensors each one consisting of a two-electrode setup (working electrode = Au, counter/reference electrode = Ag) and a well made in Plexiglas (see Figure 3b).

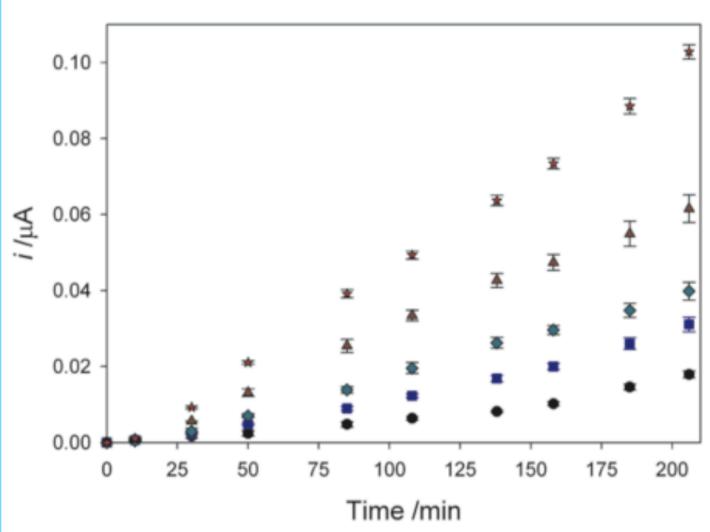

Protocol:

1) A given volume of the sample containing arsenic is mixed with a defined volume of the E. coli bioreporter suspension.

2) Immediately, 25 µL of the As(III)-E. coli solution are mixed inside the analysis well with 25 µL of 10 mM PAPG in 1x PBS (pH = 7). Final *E. coli* cells concentration $\approx 1 \times 10^8$ cells mL⁻¹.

3) Amperometric detection of PAP is started (see Figure 4).

Figure 4. Amperometry detection of PAP as a function of time for different As(III) concentrations: 0 μM (0 ppb, Filled Black Circles), 0.05 μM (3.75 ppb, Filled Blue Squares), 0.1 μM (7 ppb, Filled Cyan Diamonds), 0.2 μM (15 ppb, Filled Brown Triangles), 0.4 μM (30 ppb, Filled Red Starts). The error bars represent the calculated standard deviation from triplicates. The recorded response is proportional to the As(III) concentration.

4. QUANTIFICATION IN TAP AND GROUND WATER

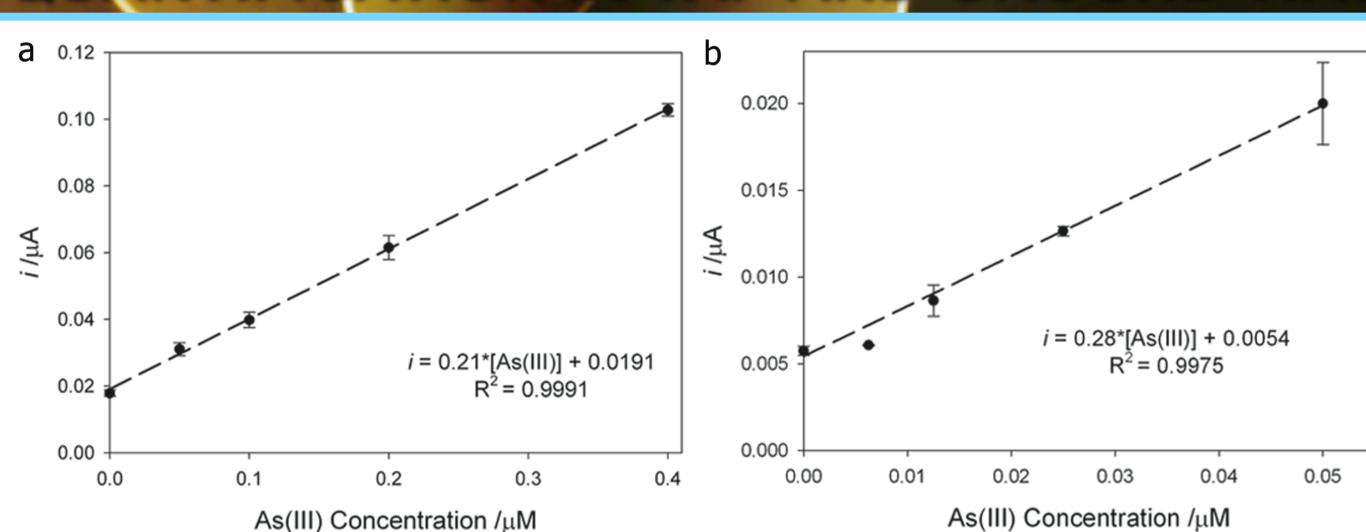


Figure 5. a) Calibration curve for As(III) at high concentration range (*i.e.* 0.05 μM to 0.4 μM or 3.75 ppb to 30 ppb) determined with the data obtained from Figure 4. b) Calibration curve for As(III) at low concentration range (i.e. 0.0125 µM to 0.05 µM or 0.94 ppb to 4 ppb) determined in a separated experiment (data not shown). LOD = 0.0105 μM or 0.8 ppb. The error bars represent the calculated standard deviation from triplicates.

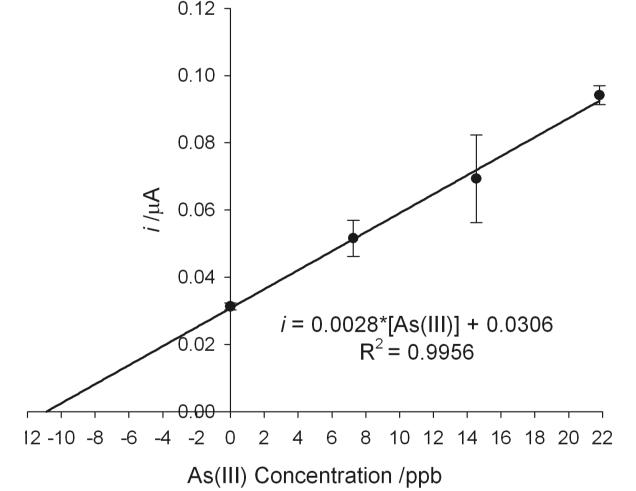


Table 1. Arsenic (III) quantification in ground water samples from Switzerland.

	As(III) Concentration /ppb	
Sample No.	Bioreporter	Reported (AAS)*
1	2.8 ± 0.4	1.9 ± 0.4
2	4.5 ± 1.6	3.8 ± 1.0
3	10.9 ± 1.2	10.4 ± 1.1

* AAS = Atomic Absorption Spectroscopy

Figure 6. Quantification of As(III) in three different samples of ground water from Switzerland employing the bacterial bioreporter by standard addition method. Only one quantification curve is shown here, but the results for all the samples are summarized in Table 1. The samples were neutralized previous to analysis with Pyrophosphate. The error bars represent the calculated standard deviation from triplicates. The response of the bacterial bioreporter is reliable for the on-site quantification of arsenic in ground water.

5. CONCLUSIONS AND PERSPECTIVES

Our results demonstrate the feasibility of coupling electrochemical and biological engineering methods for quantitative living cell toxicity detection in a high throughput microchip format. Therefore, monitoring of the water pollutant As(III) can be performed with a high selectivity and sensitivity. Indeed, the developed biochip has a limit of detection (LOD) of As(III) in potable water equal to 0.8 ppb, with a linear response in the range of concentrations tested (i.e. 1.0 ppb to 30 ppb). According to the world health organization (WHO) an As (III) concentration in potable water higher than 10 ppb represent a risk for humans, and therefore the proposed approach is a very good alternative for the portable quantification of As(III) in water samples as demonstrated by the analysis of three natural water samples from Switzerland showing a very good agreement with the reported results by AAS. Furthermore, this strategy can be extended to the analysis of other toxic agents in the environment.



References

- 1. Stocker, J.; Balluch, D.; Gsell, M.; Harms, H.; Feliciano, J.; Daunert, S.; Malik, K. A.; Van der Meer, J. R., Environ. Sci. Technol. 2003, 37 (20), 4743-4750.
- 2. Scott, D. L.; Ramanathan, S.; Shi, W.; Rosen, B. P.; Daunert, S., Anal. Chem. 1997, 69 (1), 16-20.
- 3. Popovtzer, R.; Neufeld, T.; Biran, D.; Ron, E. Z.; Rishpon, J.; Shacham-Diamand, Y., Nano Lett. 2005, 5 (6), 1023-1027.

4. Massen, M.; Liu, Z.; Haruyama, T.; Kobatake, E.; Ikariyama, Y.; Aizawa, M., Anal. Chim. Acta 1995, 304 (3), 353-359.

